Installation and Operation Instructions

Model 165-003 Blood Drawing Chair with Rotational Arms
Model 165-004 Blood Drawing Chair with Drawer and Rotational Arms

Mounting the Drawer Assembly to the Chair.

NOTE
All references to left and right are from the **patient's position** while seated in the chair. The drawer can be mounted on the left or right side of the chair.

1. Slide open the drawer assembly and remove the 3/16 inch allen wrench and nameplate.

NOTE
When the drawer assembly is to be mounted on the patient's left side, remove the mounting screws and reposition them on the left side mounting bracket and remove the screw located in the back mounting hole.

NOTE
A separate nameplate is supplied in order to cover the drawer mounting holes that will not be used. The nameplate can be found inside the drawer.

2. After determining which side the drawer (1) will be mounted to the chair, place the nameplate (2) in position over the mounting holes that will not be used on the drawer.

3. Secure the nameplate (2) to the drawer assembly with two #6-32 hex nuts (3).

4. Remove the allen head screw (4) located in the front mounting hole on the right side mounting bracket (A) of the drawer unit (1).

5. Loosen the other three mounting screws (5) on the mounting bracket (A) until there is approximately 5/16 inch (7.9 mm) clearance between the inside surface of the screw head and the mounting bracket.

6. Position the drawer unit assembly (1) against the support bracket (B) of the chair weldment (6) inserting the three mounting screws (5) into the slotted holes in the support bracket (B).

NOTE
Do not tighten the mounting screws in the slotted holes until aligning the final hole in the drawer bracket with the hole in the support bracket.

7. Move the drawer unit assembly (1) toward the narrow end of the slotted holes until the empty hole (C) in the drawer bracket (A) is aligned with the hole (D) in the support bracket (B).

8. Install the screw (4) in the empty hole (D), securing the drawer unit (1) to the support bracket (B) and tighten the three screws (5) in the slotted holes.

WARNING
Do not exceed 20 lbs. (9 kg) maximum weight capacity on the drawer unit assembly. Failure to stay within the weight limitations risks possible injury to the patient or user.

9. Slide the drawer (E) in and out to insure it operates smoothly.

Rotating Arm Operation

The pad on the rotating arm assemblies can be rotated and locked at a variety of angular positions. This can be accomplished by the following steps.

1. Pull and hold down on the knob (7) of the indexing plunger.

2. Rotate the padded arm (8) assembly to the desired position.

3. Release the knob (7) and slightly move the padded arm (8) side to side until the index plunger locks in place.

4. Check to insure the padded arm (8) is locked in position.

Drawer Removal

To remove the drawer from the drawer unit assembly pull outward on the drawer and lift the front of the drawer slightly to disengage the drawer from the drawer slides.

© Midmark Corporation - 1997

Care and Maintenance

Care of Upholstery

The upholstery material is resistant to most medicinal-type stains, but may be damaged by solvents and dyes. Regular care should be maintained by daily wiping with a damp cloth or sponge and periodic cleaning with a mild soap and water solution.

Any fluid spilled on the upholstery should be removed as quickly as possible.
In the case of stain, attempt to remove it with soap and water.

Care of Painted Metal Surfaces

All painted metal surfaces should be wiped with a clean soft cloth weekly and periodic applications of paste wax made to all surfaces to preserve the finished luster.

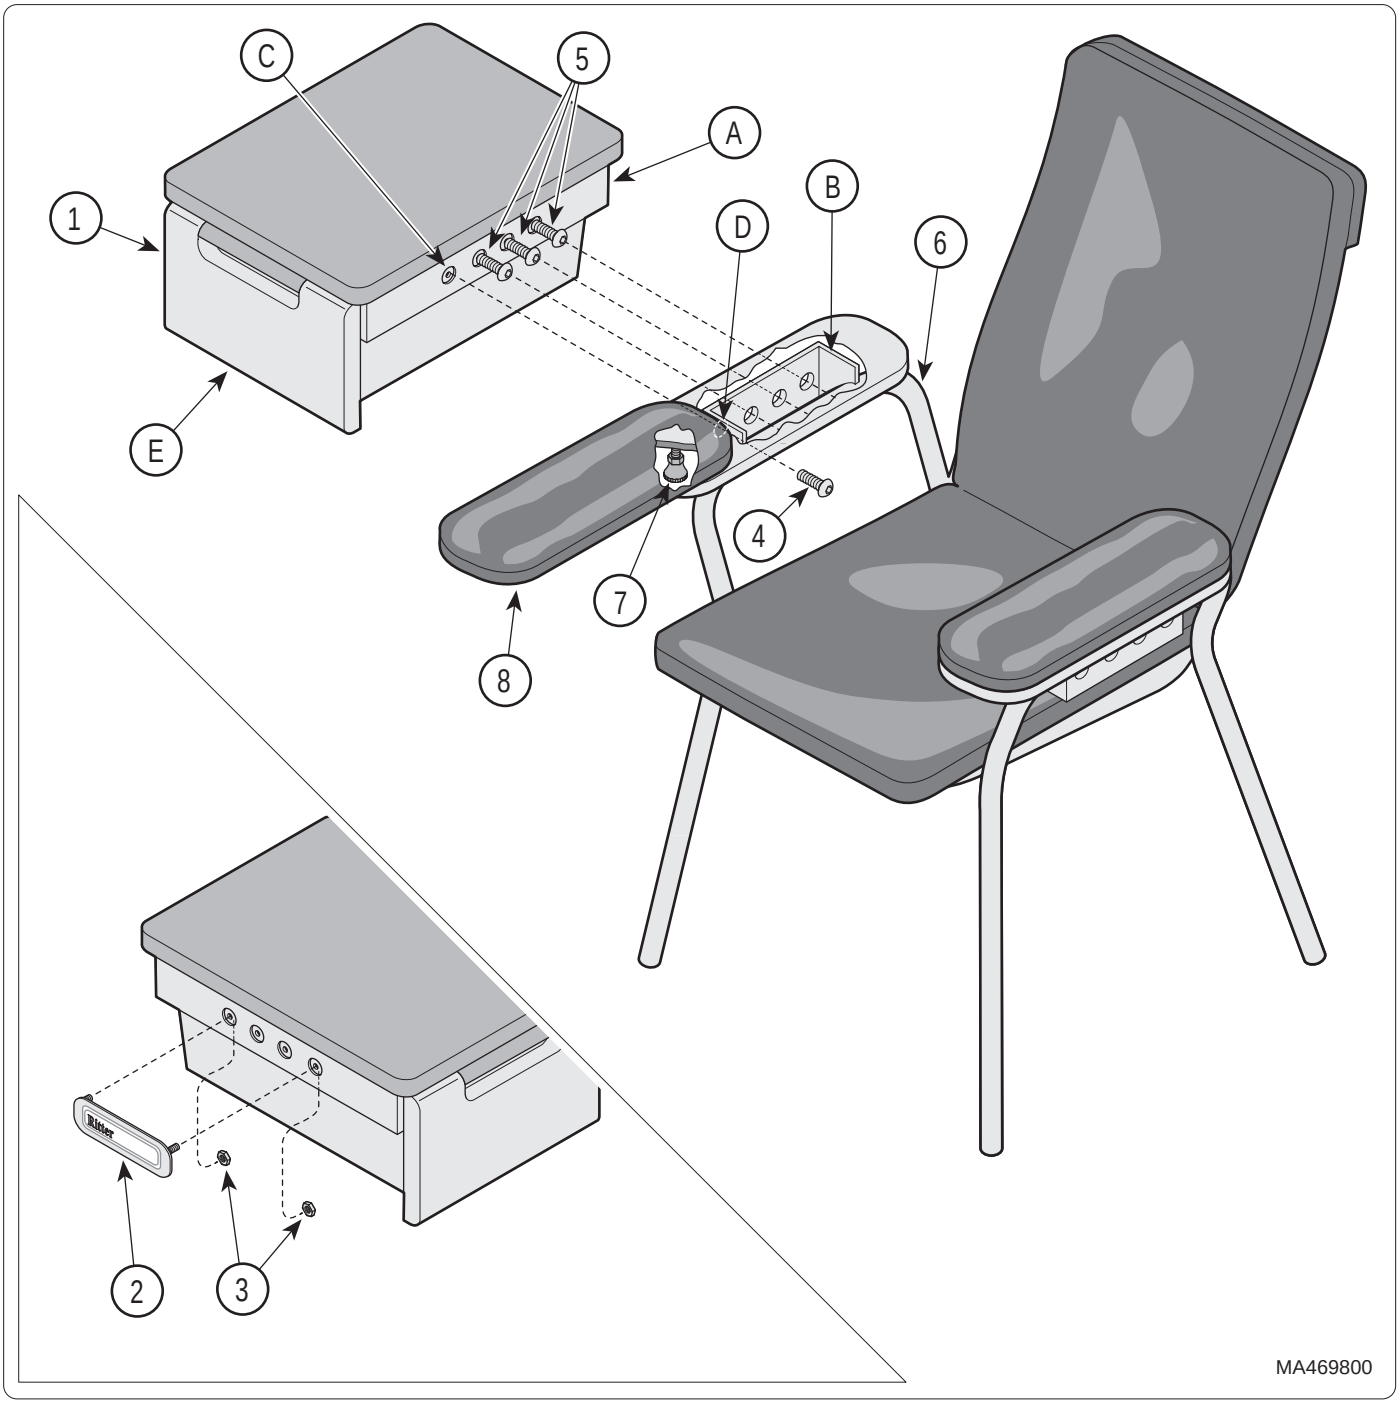

© Midmark Corporation - 1997

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
937-526-3662 TELEX 288007 FAX 937-526-5542